

Type II Collagen Detection ELISA Kit

Catalog # 6018

For Research Use Only - Not Human or Therapeutic Use

PRODUCT SPECIFICATIONS

DESCRIPTION:	ELISA kit to quantify multi-species Type II collagen
FORMAT:	96-well ELISA plate with removeable strips
ASSAY TYPE:	Sandwich ELISA
ASSAY TIME:	3.5 hours (1-step protocol) 5.5 hours (2-step protocol)
STANDARD RANGE:	200 ng/ml - 3.1 ng/ml
NUMBER OF SAMPLES:	Up to 40 (duplicate) samples/plate
SAMPLE TYPES:	Solubilized collagen and cell culture media
RECOMMENDED SAMPLE DILUTIONS:	1:1 - 1:1000
CHROMOGEN:	OPD (read at 490 nm)
STORAGE:	-20°C for 12 months
VALIDATION DATA:	Intra-assay (2.1-4.4%)/Inter-assay (6.3-9.3%)/Spiking Test (86-97%)
NOTES:	This kit has the option to run the standard and detection antibody steps in either a 1-step or 2-step procedure.

Type II Collagen Detection ELISA Kit

Catalog # 6018

For Research Use Only - Not Human or Therapeutic Use

INTRODUCTION

Type II collagen is unique among the collagen family, and its tissue distribution is limited to avascular tissues such as cartilage and the vitreous body of the eye. As type II collagen can induce arthritis in experimental animals, autoimmunity to type II collagen is suspected in the pathogenesis of certain autoimmune diseases in humans such as rheumatoid arthritis (RA), eye diseases associated with RA, and relapsing polychondritis, which affects specific tissues containing type II collagen. The Type II Collagen Detection ELISA Kit (Cat # 6018) is designed to quantify the amount of solubilized native type II collagen from various species such as human, monkey, porcine, bovine, rat, mouse, rabbit, equine, dog, and chick in cell culture samples or tissue specimens by ELISA (Table 2). This kit has the option to run the standard and detection antibody steps in a 1- or 2-step procedure (Assay Outline). Chondrex, Inc. recommends running the 1-step protocol to save time. However, the 2-step assay protocol follows the same protocol as that of Chondrex, Inc's Type I Collagen Detection ELISA kits and both protocols yield comparable standard curves and identical sample results for this kit (Figure 1). Please use the appropriate protocol best suited for your studies.

KIT COMPONENTS

Item	Quantity	Amount	Storage
Type II Collagen Standard (9034)	1 vial	100 μ l, 100 μ g/ml	-20°C
Capture Antibody (60182)	1 vial	100 μ l, 5 mg/ml	-20°C
Detection Antibody (60183)	1 vial	Lyophilized	-20°C
Solution A - Coating Buffer (9052)	1 bottle	10 ml	-20°C
Solution B - Sample/Standard Dilution Buffer (9053)	1 bottle	50 ml	-20°C
Solution C - Detection Antibody Dilution Buffer (9054)	1 bottle	10 ml	-20°C
Solution D - Streptavidin Peroxidase Dilution Buffer (9055)	1 bottle	20 ml	-20°C
Streptavidin Peroxidase (9029)	2 vials	50 μ l	-20°C
OPD (90021)	2 vials	Lyophilized	-20°C
Chromogen Dilution Buffer (90022)	1 bottle	20 ml	-20°C
Stop Solution - 2N Sulfuric Acid (9016)	1 bottle	10 ml	-20°C
Wash Buffer, 20X (9005)	1 bottle	50 ml	-20°C
ELISA Plate	1 each	96-well (8-well strips x 12)	-20°C

SOLUBILIZING COLLAGEN

For determining collagen content in cultured cell layers and tissues by ELISA, solubilizing collagen is required. For tissue specimens, a limited digestion with pepsin is highly recommended for native collagen preparation as other neutral proteinases, such as pronase and papain, digest collagen into small peptides. Pepsin only digests telopeptides located on both the N- and C-terminals of the collagen molecule and is not capable of digesting the helical conformation region of the collagen molecule itself. Please inquire with Chondrex, Inc. customer service for "Tips on Solubilization of Collagen".

Solubilizing collagen from tissues by limited pepsin digestion (generally collagen to pepsin ratio is 100:1) depends on the types of tissues and the contents of the intra- and inter-molecular cross-linkages. For example, bone and Achilles tendon are resistant to pepsin digestion and only 10-20% of the collagen tissue will be solubilized. Young calf skin collagen will be completely solubilized by pepsin digestion within 24-48 hours, while it takes 7-9 days to solubilize adult skin. Pepsin resistant insoluble collagen might be solubilized by alkaline treatment. Suspend insoluble collagen in cold 0.1N NaOH solution containing 10% Na₂SO₄ and 0.1M Amine such as Tris and incubate at 4°C for 1-2 weeks. After treatment of collagen with alkaline, neutralize the pH to 5.0 with HCl, and then dilute it with 0.05M acetic acid or neutral buffer such as 0.1M Tris-0.3M NaCl, pH 7.5.

Therefore, the optimum solubilization condition for individual samples should be determined before processing samples. Collagen can be analyzed by 6% SDS-gel under non-reducing conditions, using authentic type I collagen as a standard. If samples contain bands larger than the γ -chain (MW = 300 Kd), the samples must be further digested by pepsin or elastase which will digest the intra- and inter-collagen cross-linkages. On the other hand, if smaller bands or smear bands are observed under the α -chain (MW = 100 Kd), the samples might be over-digested. Therefore, it is critical to understand the biological and physico-chemical properties of individual collagen samples.

NOTES BEFORE USING ASSAY

NOTE 1: It is recommended that the standard and samples be run in duplicate.

NOTE 2: Warm up all buffers to room temperature before use.

NOTE 3: Crystals may form in Wash Buffer, 20X when stored at cold temperatures. If crystals have formed, warm the wash buffer by placing the bottle in warm water until crystals are completely dissolved.

NOTE 4: Measure exact volume of buffers using a serological pipet, as extra buffer is provided.

NOTE 5: Cover the plate with plastic wrap or a plate sealer after each step to prevent evaporation from the outside wells of the plate.

NOTE 6: For partial reagent use, please see the assay protocol's corresponding step for the appropriate dilution ratio. For example, if the protocol dilutes 50 μ l of a stock solution in 10 ml of buffer for 12 strips, then for 6 strips, dilute 25 μ l of the stock solution in 5 ml of buffer. Partially used stock reagents may be kept in their original vials and stored at -20°C for use in a future assay.


NOTE 7: This kit contains animal components from non-infectious animals and should be treated as potential biohazards in use and for disposal.

1-STEP ASSAY PROCEDURE

- Add Capture Antibody:** Dilute one vial of Capture Antibody with 10 ml of Coating Buffer (Solution A). Alternatively, dilute according to the table below. Add 100 μ l of capture antibody solution to each well and incubate at 4°C overnight. Any remaining Capture Antibody Stock Solution can be stored at -20°C for future use.

Strip #	Capture Antibody (μ l)	Solution A (ml)
2	17	1.7
4	33	3.3
6	50	5.0
8	66	6.6
10	82	8.2
12	100	10.0

- Prepare Standard Dilutions:** The standard range is 3.1-200 ng/ml. Prepare serial dilutions of the standard by mixing 20 μ l of 100 μ g/ml standard with 980 μ l of Sample/Standard Dilution Buffer (Solution B) to make a 2,000 ng/ml stock solution. Mix 100 μ l of the 2,000 ng/ml stock solution with 900 μ l of Solution B to make a 200 ng/ml standard stock solution. Then serially dilute it with Solution B. For example, mix 250 μ l of the 200 ng/ml standard stock solution with an equal volume of Solution B to make a 100 ng/ml standard stock solution and repeat it five more times for 50, 25, 12.5, 6.3, and 3.1 ng/ml standard stock solutions. The original standard stock solution may be stored at -20°C for use in a future assay. Chondrex, Inc. recommends making fresh serial dilutions for each assay.

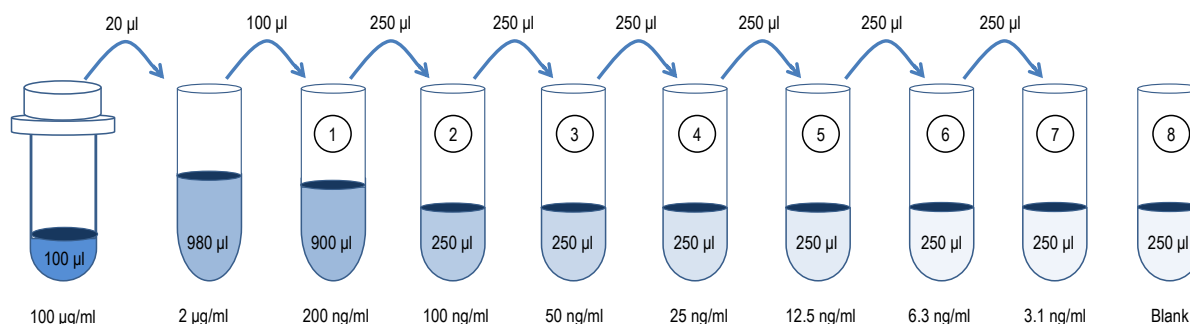

- Prepare Sample Dilutions:** Dilute tissue samples 1:1-1:1000 with Solution B depending on the estimated collagen content in the samples. The samples must be diluted with Solution B to maintain optimal assay conditions.

NOTE: Cell samples and culture media can be assayed at a 1:1 dilution with Solution B.

- Prepare Detection Antibody:** Dissolve one vial of Detection Antibody in 5 ml Detection Antibody Dilution Buffer (Solution C). Alternatively, dissolve one vial of Detection Antibody in 50 μ l of Solution C and dilute accordingly.

Strip #	Detection Antibody (μ l)	Solution C (ml)
2	8	0.8
4	17	1.7
6	25	2.5
8	33	3.3
10	42	4.2
12	50	5.0

5. **Dilute Wash Buffer:** Dilute 50 ml of 20X wash buffer in 950 ml of distilled water (1X wash buffer). Wash the plate with 1X wash buffer at least 3 times using a wash bottle with manifold or an automated plate washer. Empty the plate by inverting it and blotting on a paper towel to remove excess liquid. *Do not allow the plate to dry out.*
6. **Add Standards, Samples, and Detection Antibodies:** Add 50 μ l of standards, Solution B (blank), and samples to appropriate wells in duplicate. Add 50 μ l of detection antibody solution to all wells. Incubate at room temperature for 2 hours.
7. **Wash:** Wash the plate with 1X wash buffer at least 3 times using a wash bottle with manifold or an automated plate washer. Empty the plate by inverting it and blotting on a paper towel to remove excess liquid. *Do not allow the plate to dry out.*
8. **Add Streptavidin Peroxidase:** Dilute one vial of Streptavidin Peroxidase in 10 ml of Streptavidin Dilution Buffer (Solution D). Add 100 μ l of streptavidin peroxidase solution to each well and incubate at room temperature for 1 hour.

Strip #	Streptavidin Peroxidase (μ l)	Solution D (ml)
2	8	1.7
4	17	3.3
6	25	5.0
8	33	6.6
10	42	8.2
12	50	10.0


9. **Wash:** Wash the plate with 1X wash buffer at least 3 times using a wash bottle with manifold or an automated plate washer. Empty the plate by inverting it and blotting on a paper towel to remove excess liquid. *Do not allow the plate to dry out.*
10. **Add OPD:** Dissolve one vial of OPD with 10 ml of Chromogen Dilution Buffer just prior to use. Add 100 μ l of OPD solution to each well immediately after washing the plate and incubate for 30 minutes at room temperature.
11. **Stop:** Add 50 μ l of 2N sulfuric acid (Stop Solution) to each well.
12. **Read Plate:** Read the OD values at 490 nm. If the OD values of samples are greater than the OD values of the highest standard, re-assay the samples at a higher dilution. A 630 nm filter can be used as a reference.

2-STEP ASSAY PROCEDURE

- Add Capture Antibody:** Dilute one vial of Capture Antibody with 10 ml of Coating Buffer (Solution A). Alternatively, dilute according to the table below. Add 100 μ l of capture antibody solution to each well and incubate at 4°C overnight. Any remaining Capture Antibody Stock Solution can be stored at -20°C for future use.

Strip #	Capture Antibody (μ l)	Solution A (ml)
2	17	1.7
4	33	3.3
6	50	5.0
8	66	6.6
10	82	8.2
12	100	10.0

- Prepare Standard Dilutions:** The standard range is 3.1-200 ng/ml. Prepare serial dilutions of the standard by mixing 20 μ l of 100 μ g/ml standard with 980 μ l of Sample/Standard Dilution Buffer (Solution B) to make a 2,000 ng/ml stock solution. Mix 100 μ l of the 2,000 ng/ml stock solution with 900 μ l of Solution B to make a 200 ng/ml standard stock solution. Then serially dilute it with Solution B. For example, mix 250 μ l of the 200 ng/ml standard stock solution with an equal volume of Solution B to make a 100 ng/ml standard stock solution and repeat it five more times for 50, 25, 12.5, 6.3, and 3.1 ng/ml standard stock solutions. The original standard stock solution may be stored at -20°C for use in a future assay. Chondrex, Inc. recommends making fresh serial dilutions for each assay.

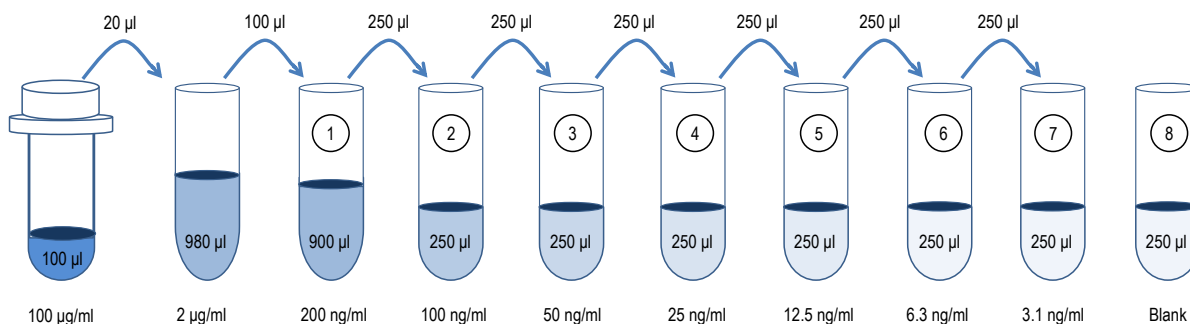

- Prepare Sample Dilutions:** Dilute tissue samples 1:1-1:1000 with Solution B depending on the estimated collagen content in the samples. The samples must be diluted with Solution B to maintain optimal assay conditions.

NOTE: Cell samples and culture media can be assayed at a 1:1 dilution with Solution B.

- Dilute Wash Buffer:** Dilute 50 ml of 20X wash buffer in 950 ml of distilled water (1X wash buffer). Wash the plate with 1X wash buffer at least 3 times using a wash bottle with manifold or an automated plate washer. Empty the plate by inverting it and blotting on a paper towel to remove excess liquid. *Do not allow the plate to dry out.*
- Add Standards and Samples:** Add 100 μ l of standards, Solution B (blank), and samples to appropriate wells in duplicate. Incubate at room temperature for 2 hours.
- Wash:** Wash the plate with 1X wash buffer at least 3 times using a wash bottle with manifold or an automated plate washer. Empty the plate by inverting it and blotting on a paper towel to remove excess liquid. *Do not allow the plate to dry out.*
- Prepare Detection Antibody:** Dissolve one vial of Detection Antibody in 10 ml Detection Antibody Dilution Buffer (Solution C). Alternatively, dissolve one vial of Detection Antibody in 50 μ l of Solution C and dilute accordingly. Add 100 μ l of detection antibody solution to all wells. Incubate at room temperature for 2 hours.

Strip #	Detection Antibody (μ l)	Solution C (ml)
2	8	1.7
4	17	3.3
6	25	5.0
8	33	6.6
10	42	8.2
12	50	10.0

8. **Wash:** Wash the plate with 1X wash buffer at least 3 times using a wash bottle with manifold or an automated plate washer. Empty the plate by inverting it and blotting on a paper towel to remove excess liquid. *Do not allow the plate to dry out.*
9. **Add Streptavidin Peroxidase:** Dilute one vial of Streptavidin Peroxidase in 10 ml of Streptavidin Dilution Buffer (Solution D). Add 100 μ l of streptavidin peroxidase solution to each well and incubate at room temperature for 1 hour.


Strip #	Streptavidin Peroxidase (μ l)	Solution D (ml)
2	8	1.7
4	17	3.3
6	25	5.0
8	33	6.6
10	42	8.2
12	50	10.0

10. **Wash:** Wash the plate with 1X wash buffer at least 3 times using a wash bottle with manifold or an automated plate washer. Empty the plate by inverting it and blotting on a paper towel to remove excess liquid. *Do not allow the plate to dry out.*
11. **Add OPD:** Dissolve one vial of OPD with 10 ml of Chromogen Dilution Buffer just prior to use. Add 100 μ l of OPD solution to each well immediately after washing the plate and incubate for 30 minutes at room temperature.
12. **Stop:** Add 50 μ l of 2N sulfuric acid (Stop Solution) to each well.
13. **Read Plate:** Read the OD values at 490 nm. If the OD values of samples are greater than the OD values of the highest standard, re-assay the samples at a higher dilution. A 630 nm filter can be used as a reference.

CALCULATING RESULTS

1. Average the duplicate OD values for the blank (B), standards, and test samples.
2. Subtract the averaged blank OD values from the averaged OD values of the standards and test samples.
3. Plot the OD values of standards against the concentration of standards (ng/ml). Using a log/log plot will linearize the data. Figure 1 shows a representative experiment where the standard range is 3.1 - 200 ng/ml and the 1-step protocol and 2-step protocol are compared.
4. The ng/ml of collagen in test samples can be calculated using regression analysis. Multiply it by the sample dilution factor to obtain the collagen concentration (ng/ml) in the original sample specimens.

Figure 1 - Typical Standard Curves for the Type II Collagen Detection ELISA Kit

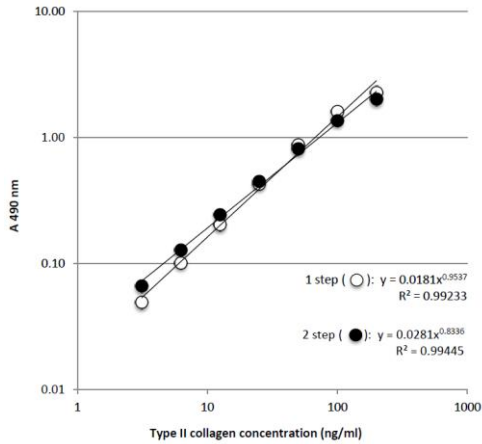

Standard (ng/ml)	1-Step (OD)	2-Step (OD)
200	2.278	2.007
100	1.597	1.353
50	0.876	0.809
25	0.427	0.447
12.5	0.203	0.243
6.3	0.101	0.127
3.1	0.049	0.066

ASSAY VALIDATION

Table 1 - Reproducibility Data for the Type II Collagen Detection ELISA Kit

Test	5 ng/ml	25 ng/ml	100 ng/ml
Intra-Assay CV (%)	4.4	2.2	2.1
Inter-Assay CV (%)	9.3	6.8	6.3
Spike Test* (%)	86%	97%	97%

* Known amounts of type II collagen were added to standards and then diluted with Solution B.

Table 2 - Reactivity of Type II collagen from various species assayed by the Type II Collagen Detection ELISA Kit.

Species	Chick	Human	Mouse	Rat	Bovine	Porcine
Cross-reactivity	100%	91%	98%	103%	247%	121%

TROUBLESHOOTING

For frequently asked questions about assays and ELISAs, please see Chondrex, Inc.'s [Assay FAQ](#) for more information.